



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Fun In The Country Alpacas/Kimberly Les
10337 Washburn Road
Columbiaville MI 48421 USA

02/25/20

Test No: 987345


Animal and Sample Description

Animal Name: Elita
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 32512397
Sample Location: Side
Sample Date: 04/19/19
Age: 09/15/12

Laboratory Data

| | | | |
|--|--------------|---------------------------------|--------------|
| Mean Fiber Diameter: | 18.4 microns | Spin Fineness: | 17.7 microns |
| Standard Deviation: | 3.6 microns | Medullated Fibers: | 0.0 % |
| Coefficient of Variation: | 19.6 % | Mean Curvature (deg/mm): | 42.3 |
| Fibers Greater Than 30 microns: | 0.9 % | SD Curvature (deg/mm): | 26.0 |

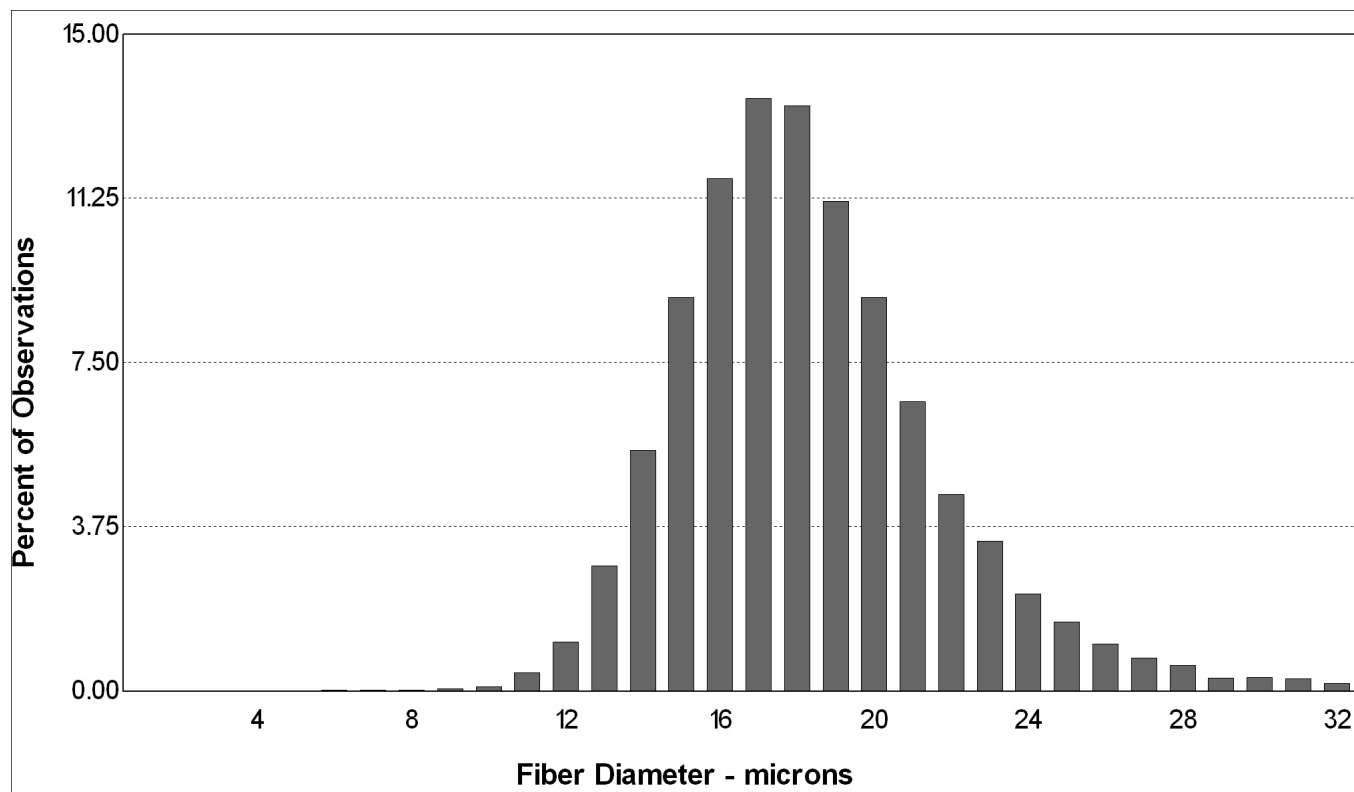

This Test Performed According to I.W.T.O Method 47